


Difference spectrum and model fit

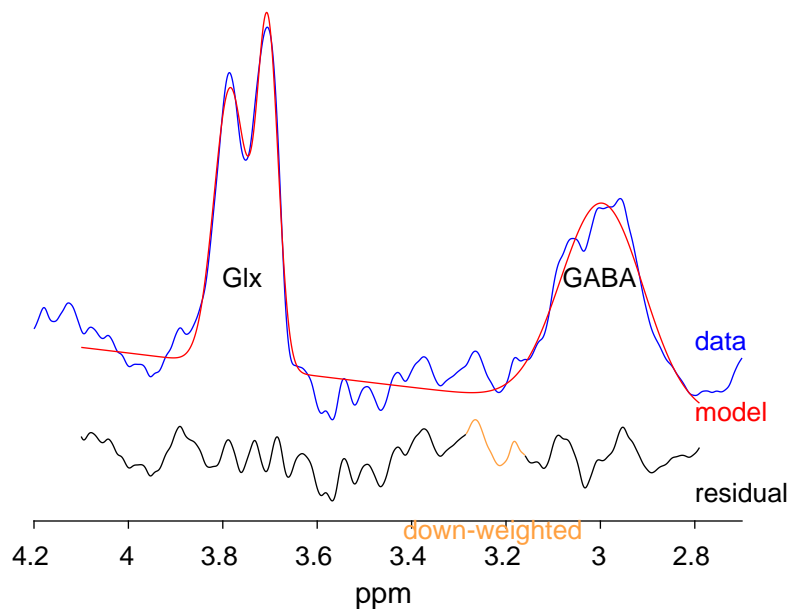

Filename: meas_MID00158_FID37598_ej...
a_svs_mpress_ACC_Met_1.dat

Area

GABA+: 0.000563
Glx: 0.000536
Water: 10.7
Cr: 0.00691

Linewidth

Water: 10.74 Hz
Cr: 8.81 Hz

SNR

Water: 33160
Cr: 318

Fit error

GABA+,Water: 6.66%
GABA+,Cr: 6.72%
Glx,Water: 4.05%
Glx,Cr: 4.14%

Quantification

GABA+/Water: 1.88 i.u.
GABA+/Cr: 0.08
Glx/Water: 6.61 i.u.
Glx/Cr: 0.08
FitVer: 230622

Reference signals

