




**Edited Spectra
(pre- and post-alignment)**

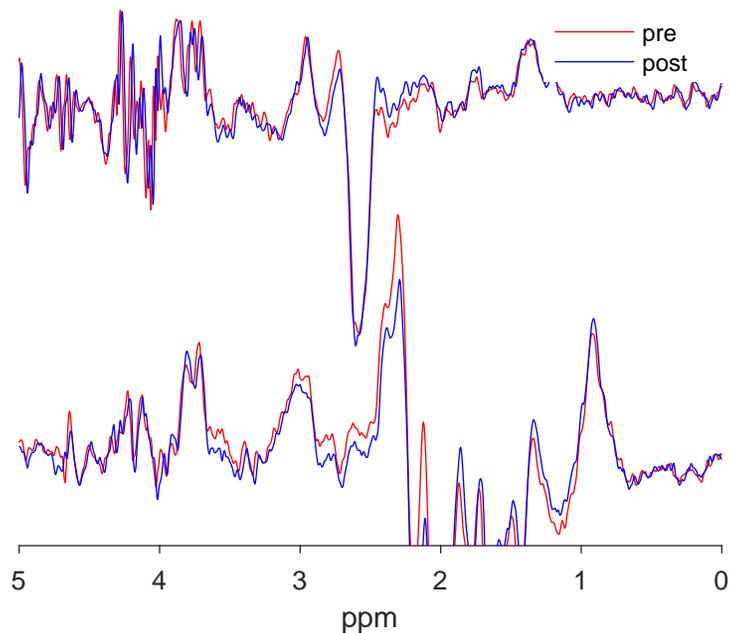

Cr Frequency

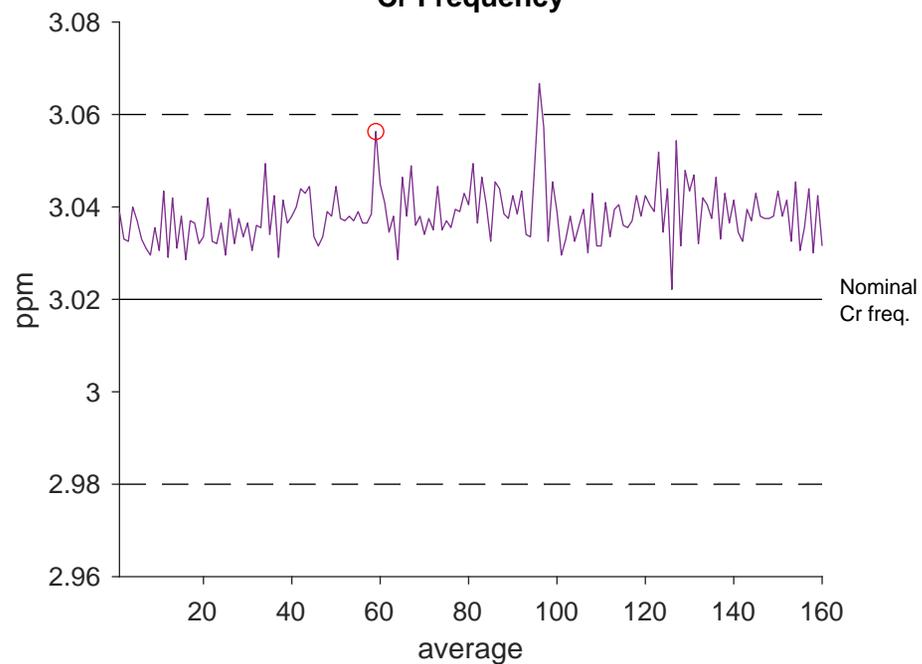

**Cr Frequency
(pre- and post-alignment)**

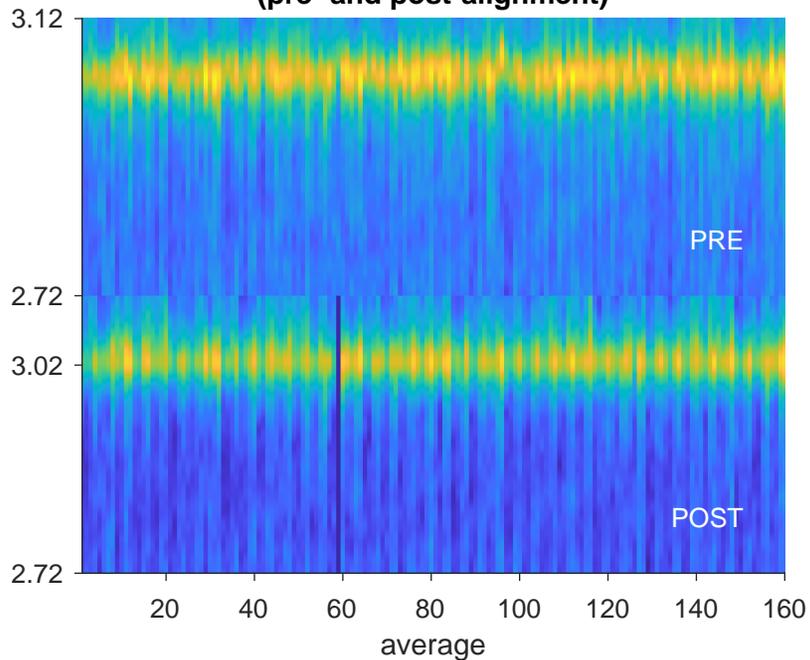

Filename: meas_MID00296_FID17977_HERMES_...
N_{avg}: 160 averages
Volume: 27 mL
Alignment: SpecRegHERMES
LB: 3 Hz
Rejects: 1
LoadVer: 200226

