


## Difference Spectrum and Model Fit

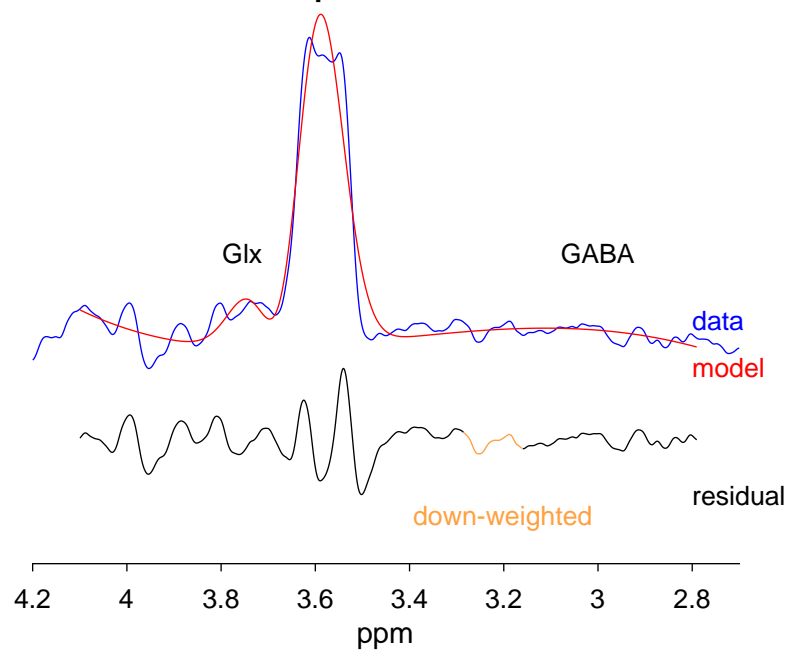

Filename: P45056.7

**Area**

GABA+: 0.00223

Glx: 5.47e-06

Water: 0.206

Cr: 3.53e-05

**Linewidth**

Water: 5.37 Hz

Cr: 5.95 Hz

**SNR**

Water: 498496

Cr: 65

**Fit Error**

GABA+,Water: 0.64%

GABA+,Cr: 22.84%

Glx,Water: 0.57%

Glx,Cr: 22.84%

**Quantification**

GABA+/Water: 411.30 i.u.


GABA+/Cr: 63.19

Glx/Water: 3.41 i.u.

Glx/Cr: 0.15

FitVer: 210405

## Reference Signals

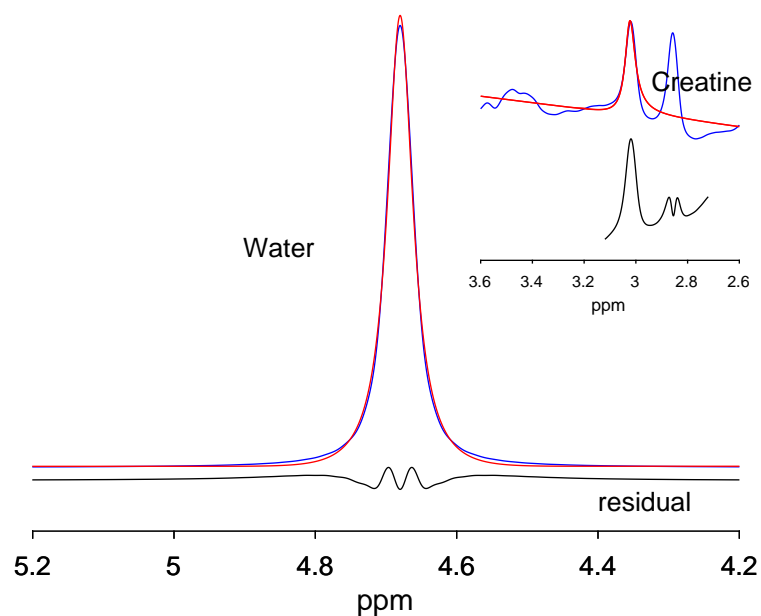

3.2.0